

Contents

1. Background	4
2. Revision History	4
3. Conventions	4
3.1 Abbreviations etc	4
3.2 Document Structure.....	4
4. System Description	4
4.1 Context and Purpose.....	4
4.2 Configurations.....	5
5. Functional Requirements.....	6
5.1 General requirements	6
5.2 Wrist Joint Function, WJF.....	8
5.3 Wrist Motor Function, WMF.....	8
5.4 Wrist Servo Function, WSF.....	9
5.5 Wrist Communication Function, WCF.....	10
5.6 Wrist Power Function, WPF	11
5.7 Proximal Attachment Function, PAF	12
5.8 Distal Attachment Function, DAF.....	12
Bibliography	14

List of Figures

Figur 1 System context.....	5
Figur 2 The two different equipment configurations	6

1. Background

The functionally optimal 1-DOF wrist prosthesis kinematics was theoretically derived in (Stavdahl, 2002). Now one aims at implementing a physical device based on these principles. The current document constitutes a functional specification for this device, which covers not only the kinematics but even mechanical, electrical, electronic and algorithmic aspects.

2. Revision History

When	Who	What
2005.02.08	Ø.Stavdahl	Brief revisions for FPGA-based version. Several requirements and comments clarified and typos fixed. This relates to: GEN-08, WJF-01, WJF-02, WJF-03, WSF-01-03, WSF-03, WCF-02, WCF-03, WCF-04, WCF-04-01, WCF-05, WCF-09, WCF-10, WPF-02, WPF-03, Circuit board geometry included.
Spring 2010	Inge Brattbakken	Revised specifications regarding communication. This relates to WCF-02 and WCF-03. Also removed requirements no longer relevant. Those being: WCF-04, WCF-04-01, WCF-04-02, WCF-06, WCF-08 and WCF-09.

3. Conventions

3.1 Abbreviations etc

The following conventions apply to this document:

NA	Not Applicable; irrelevant
HW	Hardware
SW	Software
TBC	To Be Completed; an aspect that has to be filled in.
TBD	To Be Defined; an aspect that is still not completely defined.

Use of the word *shall* denotes requirements that must be met by the system, while the word *should* denotes requirements that are desirable and must be met unless justification is provided for an alternative.

3.2 Document Structure

TBC.

4. System Description

4.1 Context and Purpose

The “system” referred to here is the entire wrist prosthesis, including both mechanical, electrical/electronic and

software components. The primary purpose of the system is to rotate/orient the terminal device with respect to the forearm according to user input. Figure 1 gives an overview of the system and its context.

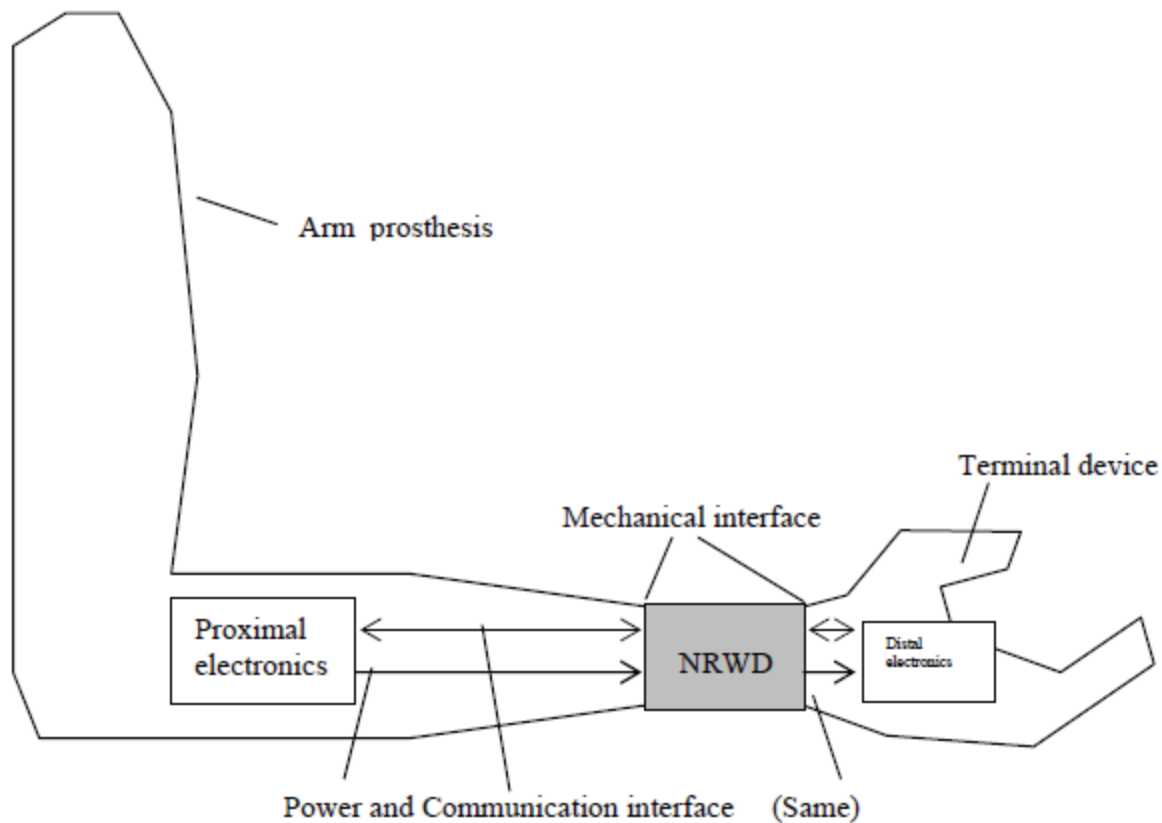



Figure 1 System context

The proximal electronics includes a battery pack or another electric power source, as well as digital circuits with sensors for reading the user's motor intent (typically EMG electrodes, switches, "pressure pads" or the like) and communication of this intent to the joint controllers in the prosthesis. While the figure suggests that the proximal electronics is situated in the forearm, this needs not be the case; in the case of a total arm replacement the prosthesis may comprise motorized shoulder, elbow, wrist and/or finger functions, and the arm electronics may correspondingly be distributed in the different parts of the arm. The "Proximal electronics" box Figure 1 thus represents all the electronics proximal to the wrist, while the "Distal electronics" represents any or all electronic components distal to the wrist, such as a motor controller responsible for opening and closing of the hand.

4.2 Configurations

The system is applicable to several different equipment configurations, as indicated in Figure 2. These configurations include the following, listed in the order of relevance and only the first two being absolutely necessary to implement:

1. A completely digital mode where all intercomponent communication is based on a data bus. This mode is for use with other novel systems that support the same communication protocol.
2. A hybrid mode where the proximal communication (i.e. between the wrist and proximal electronics) is analog while the distal communication is digital. This is for using a novel hand in systems based on analog electrodes and the like.

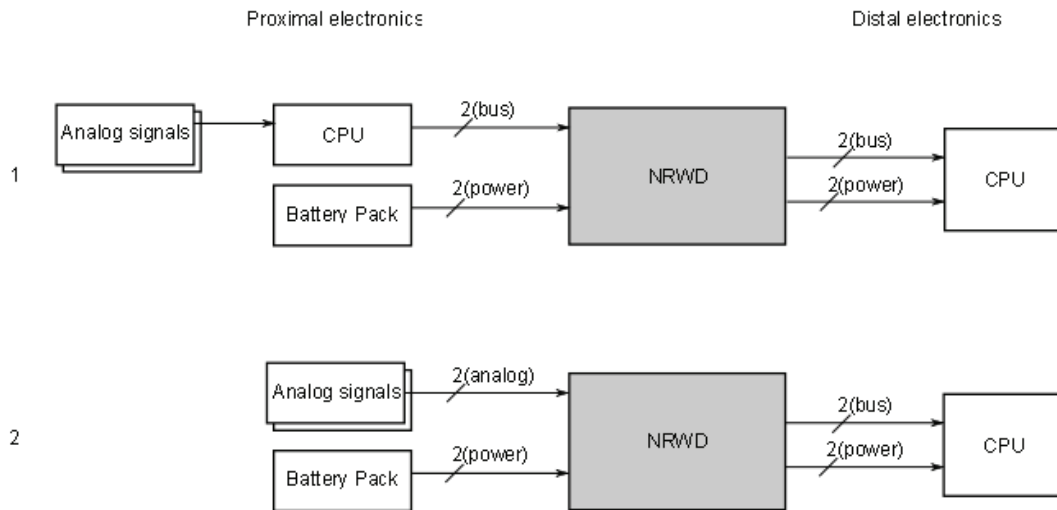

Figur 2 The two different equipment configurations

5. Functional Requirements


5.1 General requirements

The NRWD system shall implement the following functions and satisfy the following requirements.

Req. no.	Description	Comments
GEN-01	A joint which implements the optimal kinematics described in (Stavdahl, 2002) – Wrist Joint Function, WJF.	
GEN-02	An electric motor which drives the movement of the joint via a gear train – Wrist Motor Function, WMF.	
GEN-03	A motor control interface and regulation process to control the movements of the WJF. – Wrist Servo Function, WSF.	
GEN-04	A communication function that interfaces with WSF and other connected systems – Wrist Communication Function, WCF.	“Other connected systems” typically include proximal and distal joint controllers, as well as units for system diagnosis and configuration.
GEN-05	A power adaptation function that enables the system to run from a variety of voltage levels – Wrist Power Function, WPF.	Compliance with commercial and research systems.

GEN-06	A mechanism for attachment of the wrist to the forearm socket. – Proximal Attachment Function, PAF.	
GEN-06-01	The PAF shall be disconnectable and, when disconnected, allow entry to the space proximal to the wrist.	For maintenance and replacement of forearm electronics.
GEN-07	A mechanism for attachment of the wrist to the terminal device – Distal Attachment Function, DAF.	
GEN-08	An outer geometry that crudely resembles that of an adult wrist – Wrist Geometry Function, WGF.	No component shall extend beyond the envelope of a normal wrist, which has an elliptic crosssectional area of approx. 5 cm x 4 cm. All parts and connectors must be kept small.
GEN-08-01	The longitudinal dimension (along the forearm) of the entire NRWD should be as short as possible, and shall not exceed 65 mm.	Allows longer residual limbs to use it, i.e. “larger market”. 65 mm is Bock spec.
GEN-09	The system should consume a minimum of energy, and the current consumption shall be kept below 2A at all times.	When motor is active, its output dictates a lower bound for the power consumption. This requirement just implies that unnecessary circuits should be turned off, and active use should be made of the controller’s various sleep modes.
GEN-10	The system shall be modular with respect to both HW and SW.	
GEN-11	The weight of the entire NRWD should not exceed 100 g.	Industrial components: Otto Bock: 96 g, VASI:100 g.

Figur 3 depicts the functions and their dependencies.

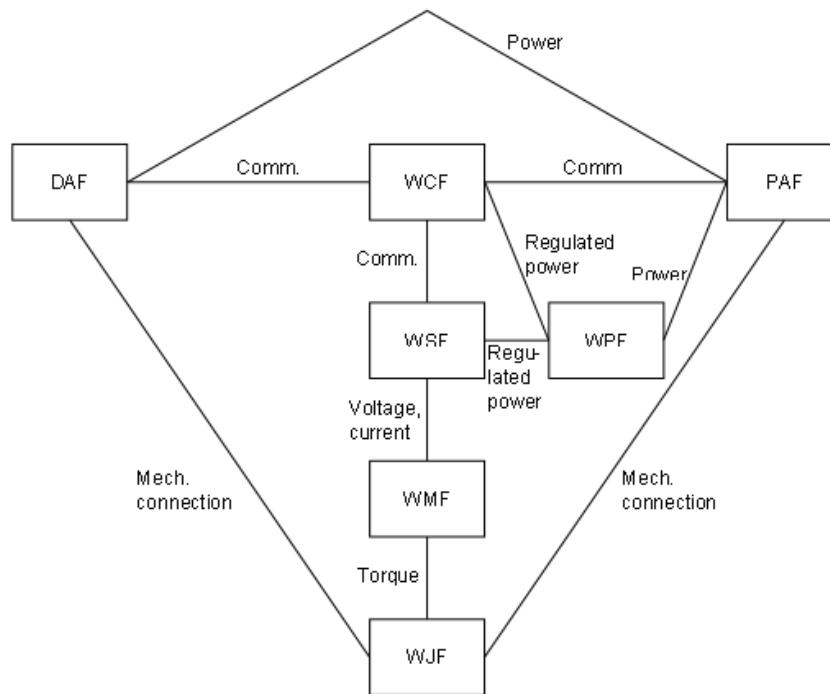

Figur 3 Functional block diagram

5.2 Wrist Joint Function, WJF

The following requirements are derived from GEN-01.

Req. no.	Description	Comments
WJF-01	The NRWD joint shall be a single, simple revolute joint which axis of rotation can be placed at an attitude with respect to the forearm and terminal device as specified in (Stavdahl, 2002) Equations (7.4) and (7.5).	Derived from (specific version of) GEN-01. Note a typographical error in Eqn. (7.5); last element of vector should read "-0.23" instead of "0.23".
WJF-02	The joint axis should be manually adjustable to other attitudes than that specified in WJF-01.	In order to test other axis alignments. Note that adjustability wrt. forearm AND hand requires TWO adjustable functions!
WJF-03	The joint shall enable an angular excursion of at least 180 degrees. The excursion should be unlimited.	180 deg is crudely that of a healthy limb.

5.3 Wrist Motor Function, WMF

The following requirements are derived from GEN-02.

Req. no.	Description	Comments
WMF-01	The wrist joint (output of the gear train) shall have a maximum angular	Otto Bock spec. No-load speed

	velocity of at least 1.4 rad/s (81 deg/s). The maximum velocity should be as high as possible.	
WMF-02	The wrist joint should have a maximum torque of at least 34,3 mNm.	VASl spec. Stall torque
WMF-03	The motor shall have a maximum mechanical output power of at least TBC W.	
WMF-04	The motor shall be protected from overheating. The protection should be implemented by hardware.	

5.4 Wrist Servo Function, WSF

The following requirements are derived from GEN-03.

Req. no.	Description	Comments
WSF-01	The movements of the wrist joint shall be controllable according to the following modes: <ol style="list-style-type: none"> 1. On/Off-mode 2. Position mode. 3. Velocity mode 	
WSF-01-01	In On/Off-mode the motor shall be at rest or run at maximum speed (open-loop) in one direction according to a given setpoint.	Requires only transistor bridge.
WSF-01-02	In position mode the joint angle shall be proportional to a given angular setpoint.	
WSF-01-02-01	The WSF shall include an absolute position sensor. This sensor shall provide no less than 10 bits resolution per revolution.	
WSF-01-03	In velocity mode the joint angular velocity shall be crudely proportional to a given velocity setpoint.	“Crudely proportional” implies that there is no explicit need for velocity feedback, the speed may be controlled in open-loop.
WSF-01-03-01	The WSF shall include a velocity sensor or estimator.	If brushless motor: use Hall elements for speed estimates.
WSF-02	The movements of the wrist joint should be controllable according to the following modes: <ol style="list-style-type: none"> 4. Torque mode 5. Impedance mode 	
WSF-02-04	In torque mode the motor torque shall be proportional to a given torque setpoint.	Torque crudely proportional with motor current, so current can be used for feedback.

WSF-02-04-01	The WSF should include means for monitoring motor current.	Also follows from GEN-09.
WSF-02-05	In impedance mode the mechanical impedance of the joint shall be determined by a given impedance setpoint.	Mech. Impedance = torque/velocity. May require strain gauge measurements etc. to “bypass” friction.
WSF-03	WSF shall provide an interface to WCF through which the modes (described in WFS-01 to WSF-02) can be selected and relevant parameters can be set, and through which WSF can report relevant state variables TBD.	Typically: Setpoints in, process values out. The precise content of this communication will be defined by a protocol specification (SCIP) TBD.

5.5 Wrist Communication Function, WCF

The following requirements are derived from GEN-04.

Req. no.	Description	Comments
WCF-01	The NRWD shall have a two-wire Proximal Communication Interface (PCI) and a two-wire Distal Communication Interface (DCI).	
WCF-02	The PCI shall be configurable so that it implements two (0V, 7.2V) analog input lines or a bidirectional two-wire CAN interface with the UNB protocol (Losier, 2009).	The 7.2V spec is approximate. For protocol, see comment re. WSF-03.
WCF-02-01	The analog input lines shall be able to sample both lines at a rate of 1 kHz. The sampling rate should be as high as 2 kHz.	EMG signals have a bandwidth of approx. 500Hz.
WCF-03	The DCI shall be configurable so that it implements two (0 V, 7.2 V) analog output lines or a bidirectional two-wire CAN interface with the UNB-protocol.	The 7.2V spec is approximate; it may be acceptable to reduce this to 5.0V.
WCF-05	The WCF shall be configurable to an all-digital mode, with the PCI and the DCI acting as bidirectional CAN bus interfaces.	Only a single CAN interface is necessary, as both PCI and DCI can be internally connected to this single interface.
WCF-07	The WCF should be configurable to a hybrid mode in which the PCI acts as two analog input lines while DCI acts as a bidirectional CAN-interface (cf. WCF-01).	
WCF-10	The WCF shall include a serial interface for downloading software and for debugging/diagnostic purposes.	Same fashion as AVR Butterfly serial programming. This requires a bootloader. Might include RS-232 and/or other proper interfaces.
WCF-08	WCF shall implement an interface to	

	WSF according to WSF-03.	
--	--------------------------	--

5.6 Wrist Power Function, WPF

The following requirements are derived from GEN-05.

Req. no.	Description	Comments
WPF-01	The WPF shall accept external power in the form of an unregulated two-wire DC supply.	Implies on-board voltage regulation.
WPF-02	The NRWD shall tolerate and run normally when powered with a voltage in the range (6 V, 12 V). The range of usable voltages should be as wide as (5 V, 18 V).	This corresponds to Otto Bock, Motion Control and other systems. Upper limit possibly to be relaxed (lowered).
WPF-03	The NRWD shall tolerate supply voltage in the range (0 V, 12 V) without exhibiting unpredictable behaviour and without getting damaged.	E.g. shutting down the controller before the voltage gets dangerously low, may otherwise damage Flash and EEPROM content etc. See comments to WPF-02.
WPF-04	The NRWD should automatically limit its motor current to a level that does not reduce the supply voltage below the interval given in WPF-02.	Low batteries => careful motor control to avoid power-down.

5.7 Proximal Attachment Function, PAF

The following requirements are derived from GEN-06 and more.

Req. no.	Description	Comments
PAF-01	The PAF shall comprise two parts, the proximal of which is adapted to be permanently attached to the forearm socket and the distal permanently attached to the wrist unit. The parts must “mate” to form a mechanically stable connection while also being detachable.	A commercially available “quick disconnect” unit may be used, but the entire mechanism must be kept as short as possible.
PAF-01-01	The proximal part of the PAF shall be hollow to allow access to the space within the socket proximally to the wrist.	Batteries and electrodes etc. is mounted here, so an opening must be present to allow maintenance and replacement of these units.
PAF-02	PAF disconnection should be possible with hand or a simple tool, e.g. a screwdriver.	
PAF-03	The PAF shall include a four-wire electric coupling, preferably mechanically integrated with the PAF itself.	GEN-04 and GEN-05. Preferably a “quick disconnect” type, optionally loose wires and a manually detachable coupling/plug.
PAF-03-01	The PAF electrical coupling shall include at least two power supply wires/contacts capable of transferring a constant current of 4A per wire.	This is the current for the wrist AND the terminal device.
PAF-03-02	The PAF electrical coupling should be rotatable without twisting the wires.	Brush rings etc. This requirement and DAF-02-02 are mutually exclusive; both are not needed!

5.8 Distal Attachment Function, DAF

The following requirements are derived from GEN-07 and more.

Req. no.	Description	Comments
DAF-01	The DAF should comprise two parts, the proximal of which is permanently attached to the wrist and the distal permanently attached to the terminal device. The parts must “mate” to form a mechanically stable connection while also being detachable.	The distal part may be a function of the terminal device, e.g. a Bock hand. No “quick disconnect” required here!
DAF-02	The DAF shall include a four-wire electric coupling, preferably mechanically integrated with the	GEN-04 and GEN-05. Preferably a “quick disconnect” type, optionally loose wires and a manually

	DAF itself.	detachable coupling/plug.
DAF-02-01	The DAF electrical coupling shall include at least two wires/contacts capable of transferring a constant current of 2 A per wire, and these wires shall be connected to the power supply wires from PAF.	This is the current that drives the terminal device. Check with Otto Bock (=1 A?); higher currents needed for more advanced/multifunction hands.
DAF-02-02	The DAF electrical coupling should be rotatable without twisting the wires.	Brush rings etc. This requirement and PAF-03-02 are mutually exclusive; both are not needed!

Bibliography

Losier, Yves. 2009. *Communication protocol for the AIF UNB hand project.* University of New Brunswick. 2009.

Stavdahl, Øyvind. 2002. *Optimal wrist prosthesis kinematics: Three-dimensional rotation statistics and parameter estimation.* Department of Engineering Cybernetics, Norwegian University of Science and Technology. 2002. PhD Thesis.

Stavdahl, Øyvind. 2002. *Functional Requirements Specification.* 2002.