

EEGlass: An EEG-Eyeware Prototype for Ubiquitous Brain-Computer Interaction

Athanasios Vourvopoulos
Department of Bioengineering
Institute for Systems and Robotics
Instituto Superior Técnico
Universidade de Lisboa
Lisboa, Portugal
athanasios.vourvopoulos@tecnico.ulisboa.pt

Evangelos Niforatos
Department of Computer Science
Norwegian University of Science and
Technology (NTNU)
Trondheim, Norway
evangelos.niforatos@ntnu.no

Michail Giannakos
Department of Computer Science
Norwegian University of Science and
Technology (NTNU)
Trondheim, Norway
michail.giannakos@ntnu.no

ABSTRACT

Contemporary Head-Mounted Displays (HMDs) are progressively becoming socially acceptable by approaching the size and design of normal eyewear. Apart from the exciting interaction design prospects, HMDs bear significant potential in hosting an array of physiological sensors very adjacent to the human skull. As a proof of concept, we illustrate EEGlass, an early wearable prototype comprised of plastic eyewear frames for approximating the form factor of a modern HMD. EEGlass is equipped with an Open-BCI board and a set of EEG electrodes at the contact points with the skull for unobtrusively collecting data related to the activity of the human brain. We tested our prototype with 1 participant performing cognitive and sensorimotor tasks while wearing an established Electroencephalography (EEG) device for obtaining a baseline. Our preliminary results showcase that EEGlass is capable of accurately capturing resting state, detect motor-action and Electrooculographic (EOG) artifacts. Further experimentation is required, but our early trials with EEGlass are promising in that HMDs could serve as a springboard for moving EEG outside of the lab and in our everyday life, facilitating the design of neuroadaptive systems.

CCS CONCEPTS

• **Hardware** → **Neural systems**.

KEYWORDS

Head-Mounted Displays, Electroencephalography, Brain-Computer Interfaces, Neuroadaptive Systems

ACM Reference Format:

Athanasios Vourvopoulos, Evangelos Niforatos, and Michail Giannakos. 2019. EEGlass: An EEG-Eyeware Prototype for Ubiquitous Brain-Computer Interaction. In *Adjunct Proceedings of the 2019 ACM International Joint Conference on Pervasive and Ubiquitous Computing and the 2019 International Symposium on Wearable Computers (UbiComp/ISWC '19 Adjunct)*, September

Permission to make digital or hard copies of all or part of this work for personal or classroom use is granted without fee provided that copies are not made or distributed for profit or commercial advantage and that copies bear this notice and the full citation on the first page. Copyrights for components of this work owned by others than ACM must be honored. Abstracting with credit is permitted. To copy otherwise, or republish, to post on servers or to redistribute to lists, requires prior specific permission and/or a fee. Request permissions from permissions@acm.org.

UbiComp/ISWC '19 Adjunct, September 9–13, 2019, London, United Kingdom

© 2019 Association for Computing Machinery.

ACM ISBN 978-1-4503-6869-8/19/09...\$15.00

<https://doi.org/10.1145/3341162.3348383>

9–13, 2019, London, United Kingdom. ACM, New York, NY, USA, 6 pages.
<https://doi.org/10.1145/3341162.3348383>

1 STATE OF THE ART

In the year 2022, over 80 million Head-Mounted Display (HMD) units are expected to ship, up from over 34 million units estimated to be sold in 2019¹. This predicted HMD proliferation is propelled by recent advances in optics and hardware miniaturization, rendering eyewear the next frontier for Wearable and Ubiquitous Computing (e.g., Google Glass Enterprise Edition², Microsoft HoloLens 2³, MagicLeap One⁴, Focals by North⁵ and Vuzix Blade⁶). Undoubtedly, an HMD uptake will actualize the vision of Augmented Reality (AR), disrupting the way we consume information and execute our daily chores [3]. From revisiting the groceries list to navigating to our destination, a plethora of daily tasks will be reshaped by AR and the unique form factor of HMDs. Except for the immense opportunities in interaction design, the HMD form factor promises an unprecedented contact potential with the human skull: the shell of our brain where the higher cognitive and perceptual processes reside.

Evidently, this “skull-contact” potential that eyewear bears could not go unnoticed. Various commercial eyewear products claim to utilize EEG (or EOG – electrooculography) and the contact points with the skull to provide so-called “neurofeedback”. For example, Narbis sunglasses⁷ utilize three electrodes, two at the back of the temples of the device touching the left and right mastoids, and one at the tip of a protruding arm that touches the top of the skull, for tracking concentration. When concentration is low, the Narbis electrochromatic lenses start darkening for inviting the user to focus more. Lowdown Focus by Smith⁸ employs a more socially acceptable design equipping a typical pair of sunglasses with silicon electrodes at the edges of the temples that touch the left and right mastoids. A companion mobile application connects to the Lowdown Focus sunglasses for collecting the readings so that one can track and increase one’s concentration levels. JINS

¹<https://www.gartner.com/en/newsroom/press-releases/2018-11-29-gartner-says-worldwide-wearable-device-sales-to-grow->

²<https://www.google.com/glass/start/>

³<https://www.microsoft.com/en-us/hololens>

⁴<https://www.magicleap.com/magic-leap-one>

⁵<https://www.bynorth.com>

⁶<https://www.vuzix.com/products/blade-smart-glasses>

⁷<http://narbis.com/company/>

⁸<https://www.smithoptics.com/us/lowdownfocus>



Figure 1: The EEGGlass prototype worn by a user.

MEME⁹ is perhaps the most prominent eyewear that employs near-skull contact for providing neurofeedback. JINS MEME utilizes two electrodes embedded in the bridge of the eyewear that touch the nasal bone to detect concentration levels by measuring the duration and the number of eye blinks via EOG [20]. More recently, a US patent was published about the design of an eyewear frame that features a flexible protrusion for holding the EEG electrodes in contact with the skull in different positions [5]. Beyond the strong commercialization interest, the combination of eyewear with EEG yields interesting niche applications in the domain of health research and Human-Computer Interaction (HCI). e-Glass is an EEG-enabled eyewear that employs an OpenBCI board and a set of electrodes across the inner side of the frame for detecting epileptic seizures [19]. PhysioHMD prototype adopts a bulky “mask” design that encases a portion of the face for hosting a wide range of physiological sensors, including EEG electrodes, capturing also facial expressions [2]. PhysioHMD is intended as a platform that informs the design of AR and Virtual Reality (VR) experiences.

On one hand, commercial approaches that combine modern eyewear with EEG (and EOG) are in general socially acceptable, but also rather limited in providing high-level information about brain activity (e.g., daily concentration levels), typically via a dedicated mobile application. Moreover, commercial “neurofeedback” products are considered “black-box” systems that utilize proprietary hardware and software. On the other hand, experimental EEG-eyewear prototypes produce fine-grained information about brain activity, while utilizing open hardware and software solutions. However, such prototypes are by default too dorky to wear outside a research lab, and cumbersome to use for extended periods of time. The EEGGlass prototype attempts to fuse the social acceptability and increased

⁹<https://jins-meme.com/en/>

Last accessed on July 3, 2019.

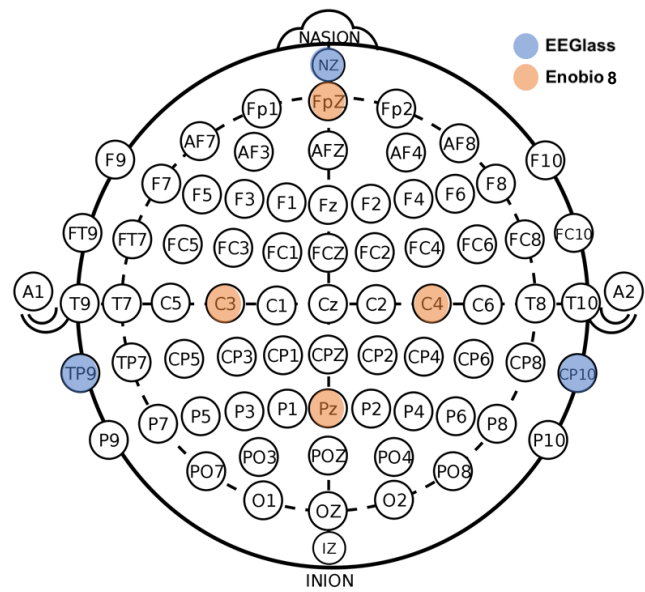


Figure 2: The 10-10 system of electrode placement topology for the EEGGlass and Enobio 8.

“wearability” of commercial EEG-eyewear with the high information granularity and openness of experimental EEG-eyewear (see Figure 1). The outcomes of such a successful fusion remain tentative but can potentially nurture existing and envisioned cognitive systems [13], democratize EEG, and eventually pave the way for touch-less input.

2 BACKGROUND

The human brain is an electrochemical system that generates a combination of dynamic biosignals or action potentials. EEG is the most common brain signal acquisition technique established almost a century ago [1]. Non-invasive EEG utilizes scalp-contact electrodes for capturing the combined electrical activity of populations of excitable cells known as neurons. When neurons activate, they produce electromagnetic fields of discrete potential patterns, distinguished by different wave oscillations in the frequency domain. These patterns are ascribed to different states of mental activity and are identified by the wave oscillations they cause in the frequency domain, known as EEG bands or rhythms [4]. EEG rhythms are divided into different frequency ranges including Delta (1–4 Hz), Theta (4–8 Hz), Alpha (8–13 Hz), Beta (13–30 Hz) and Gamma (25–90 Hz) [11], and each rhythm or combination of rhythmic activity is linked to different mental states. For example, rhythms in the Alpha and Beta frequency bands are functionally related to major sensorimotor systems, which activate primarily through motor preparation or execution [6]. Alpha and Theta oscillations are known to reflect cognitive and memory performance [9], and Theta was shown by early EEG studies to be closely connected to problem-solving, perceptual processing and learning [18]. Delta rhythm is related to concentration, attention and internal processing [8], whereas Gamma has been linked to consciousness and sense of self, and can be volitionally modulated during meditation [10].

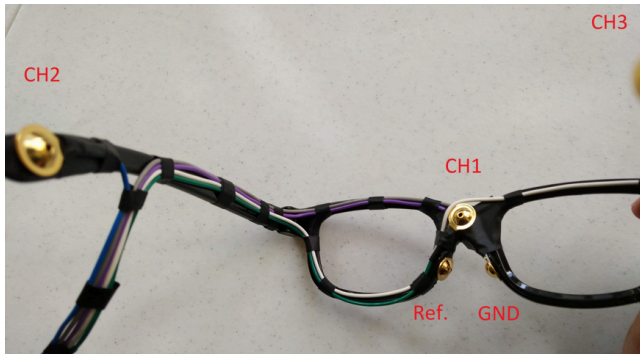


Figure 3: The EEGlasses electrode contact points and the respective OpenBCI channels.

Interpreting cognitive states or motor intentions from different EEG rhythms is a complex process and is impossible to associate a single frequency range, or cortical location, to a brain function.

Nowadays, measuring oscillatory brain activity with EEG is utilized for linking the human brain with computers via Brain-Computer Interfaces (BCIs). BCIs have been successfully utilized in the medical domain where BCIs enable amputees to gain control over prosthetic limbs [15]. Other BCI application areas include monitoring user’s cognitive states (e.g., attention levels and workload), gaming and rehabilitation. Thus, BCIs and wearable technologies such as HMDs, offer a unique opportunity to measure user needs over time and in real-life settings, informing how critical software aspects (e.g., interface) should respond or adapt. The potential of EEGlasses in monitoring surreptitiously and in real-time user’s physiological and cognitive states, renders it an ideal BCI for facilitating interaction with neuroadaptive systems.

3 EEGGLASS PROTOTYPE

The EEGlasses prototype is comprised of plastic eyewear frames that can be fitted with a Google Glass HMD. We opted for this type of eyewear for: (1) low cost, (2) availability, (3) good fitting and (4) modern HMD resemblance. In fact, the selected eyewear frames follow the trend in the field of HMDs: hardware miniaturization and social acceptability [12]. The EEG system that we embedded in the frames is Cyton Biosensing Board by OpenBCI (OpenBCI, NY, USA). OpenBCI is a popular and affordable open hardware and software platform for the collection and analysis of biosignals such as EEG, EMG (Electromyography), ECG (Electrocardiography) and others, inspired by the grassroots movement of DIY (“Do It Yourself”) [21]. The Cyton board encompasses 8 biopotential input channels (for hosting up to 8 electrodes), a 3-axes accelerometer, local storage, wireless communication modules, while being fully programmable and Arduino compatible. Evidently, the EEGlasses electrode topology is restricted by the eyewear form factor and at the contact points with the skull. Thus, EEGlasses utilizes 3 electrodes (plus 2 for reference and ground) based on the 10-10 system (see Figure 2) for measuring brain activity: 1 electrode placed inwards at the top of the eyewear bridge touching the skull at glabella, and 2 more electrodes at the inner side of the eyewear temples, touching the left and right mastoids, behind the left and right ears,



Figure 4: A user performing a motor task while wearing both EEGlasses and Enobio 8 EEG systems.

respectively (see Figure 3). The reference and ground electrodes are placed at the inner part of the eyewear bridge, touching the left and right sides of the nasal bone, respectively (see Figure 3).

4 FIRST TRIALS AND EARLY RESULTS

In this work, we explore if the low spatial resolution of a “skull-peripheral” electrode topology, imposed by the form factor of a modern HMD, can approximate the accuracy of a typical electrode topology utilized in EEG studies. To this end, we used Enobio 8 (Neuroelectronics, Barcelona, Spain) EEG system for forming a baseline. Enobio 8 is a wireless, 8-channel, EEG system with a 3-axes accelerometer for the recording and visualization of 24-bit EEG data at 500 Hz. The spatial distribution of electrodes for our trials followed the 10-10 system configuration, with electrodes placed over the frontal area (Fpz), central (C3, C4), and parietal (Pz) (see Figure 2). The electrodes were referenced and grounded to the right ear lobe, and the electrode impedance was kept at $< 20 k\Omega$. Both the Enobio 8 and the OpenBCI (embedded in the EEGlasses) EEG systems were connected via Bluetooth to a dedicated desktop computer for raw signal acquisition and processing.

The EEG acquisition session began with a 4-minute period for acquiring resting state data, and the motor-action session following next. The resting state data was acquired during alternating 1-minute periods with eyes open and eyes closed. The subject was instructed to remain silent while either fixating his eye-gaze on a white cross displayed on a computer screen, or when having his eyes closed. In the motor-action session, we employed the Graz-BCI paradigm [16] to display a random sequence of directional left and right arrows on a computer screen (see Figure 4). When an arrow appeared, the user responded to the stimulus by performing a motor-action with the corresponding hand. The motor-action session was configured to acquire data in 24 blocks (epochs) per class (left and right hand arrow).

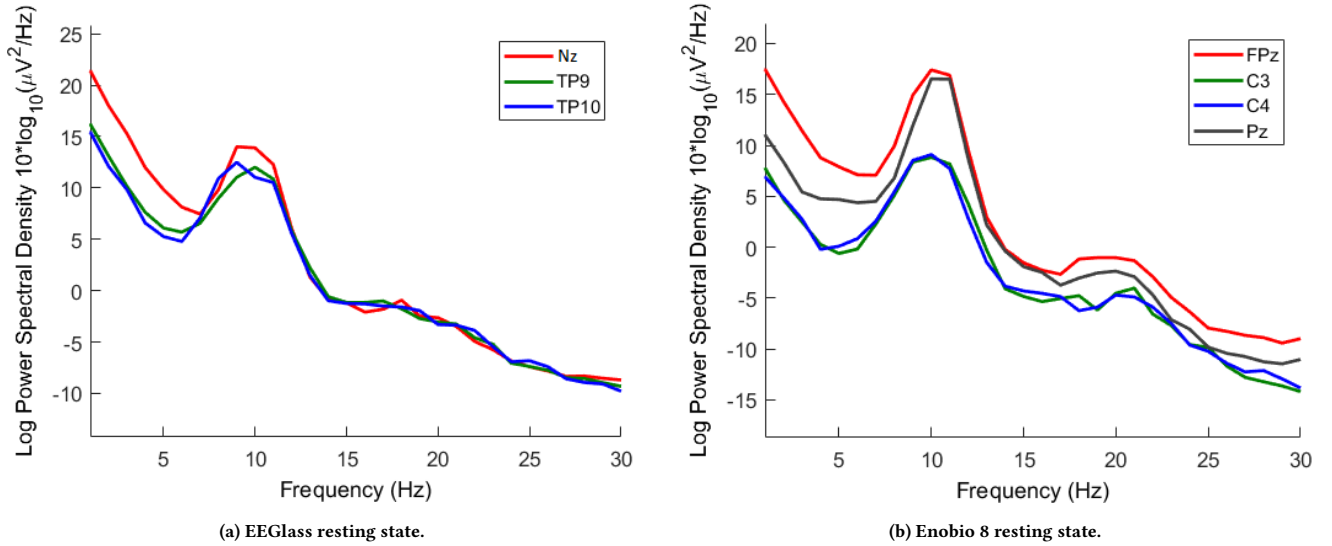


Figure 5: Resting states for EEGlass and Enobio 8. Both EEG systems detect a clear Alpha rhythm peak at 8-12 Hz.

For both systems, we used the OpenVibe acquisition servers for simultaneous EEG signal acquisition [17]. Next, we used the OpenVibe designer for obtaining the raw EEG streams from both servers and synchronizing them with the stimuli, before storing them in a .gdf file. We processed the acquired EEG signals in MATLAB® (The MathWorks, MA, USA) with the EEGLAB toolbox [7]: after importing the data and the channel information, we applied a high-pass filter at 1 Hz to remove the “baseline drift” followed by line-noise and harmonics removal at 50 Hz. Then, we used Welch’s method [22] for Power Spectral Density (PSD) of the power spectrum to compute the average spectral power across the following frequency bands during resting state: Delta (1–4 Hz), Theta (4–7 Hz), Alpha (8–12 Hz), and Beta (12–30 Hz). The event-related synchronization/desynchronization (ERS/ERD) was extracted following the standard ERS/ERD method [14] across the Alpha band power (8–12 Hz) and the Beta band power (12–30 Hz) over C3 and C4 electrode locations for the Enobio 8 system, and TP9, TP10 for the OpenBCI, respectively. We calculated the ERD by using the following formula:

$$ERD = \frac{(Power_{MotorActivity} - Power_{Baseline})}{Power_{Baseline}} * 100 \quad (1)$$

Early results from comparing EEG signals acquired via EEGlass with Enobio 8 indicate that EEGlass captures very closely the band power of Enobio 8, but also the decrease of oscillatory activity

Table 1: Resting state and EEG rhythms in $\mu V^2/Hz$ recorded by EEGlass and Enobio 8 EEG systems.

System	Delta	Theta	Alpha	Beta
EEGlass	21.279	4.775	12.992	0.431
Enobio 8	4.984	2.196	13.397	0.2993

(ERD) during the motor-action, as we anticipated. Figure 5 shows that despite the fundamentally different electrode topology of EEGlass, both EEGlass and Enobio detect a clear Alpha peak (8–12 Hz) in the electrical activity of the brain during resting state. Table 1 summarizes the recorded EEG rhythms during resting state for both EEGlass and Enobio 8 EEG systems. For investigating if brain activity linked to motor-action differed substantially between the two EEG systems, we compared the average ERD between lateral electrodes for both systems: $\Delta(TP9, C3)$ for right-hand, and $\Delta(CP10, C4)$ for left-hand movement. Dependent samples t-tests displayed significant differences in the average ERD between both pairs of lateral electrodes ($t_{TP9|C3}(199) = 10.214, p < .001$ and $t_{CP10|C4}(199), p < .001$), as shown in Figure 6 and summarized in Table 2. This indicates that the captured brain activity related to upper limb motor-action differed significantly between the EEGlass and Enobio 8 EEG systems. Moreover, Figure 7 showcases that EEGlass was able to detect basic EOG activity related to eye movement in 4 primary directions: up, down, left and right. Although the current electrode setup can capture eye-movement with only 1 degree-of-freedom (DoF), it can also detect saccadic eye movement and eye blinks.

Table 2: Average desynchronization (% ERD) between 8–24 Hz per electrode and hand for both EEGlass and Enobio 8 EEG systems.

Electrode Movement	EEGlass		Enobio 8	
	TP9 Right	TP10 Left	C3 Right	C4 Left
Mean	-5.058	-3.065	-20.272	-18.899
SD	11.6383	12.273	19.048	22.47

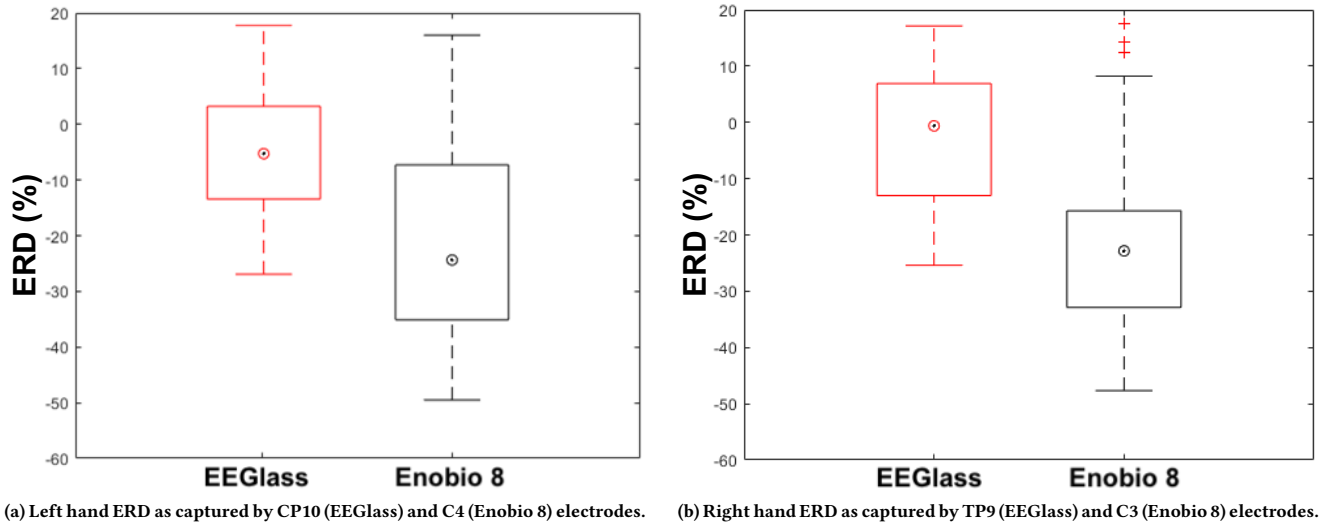


Figure 6: Average motor-action (ERD) for lateral electrode pairs of both EEGlass and Enobio 8 EEG Systems. Significant differences ($p < .001$) were found between both electrode pairs for both right and left hand motor-action.

5 DISCUSSION AND FUTURE WORK

Our preliminary results serve as a proof of concept for piggybacking EEG on eyewear and HMDs, yet in a cost-effective, unobtrusive and socially acceptable fashion. Trials with 1 participant indicate that the EEGlass is capable of capturing brain activity manifested in two modes of resting state: (a) eyes open and focused on a target, and (b) eyes closed. In fact, brain activity recorded during resting state with EEGlass demonstrates similar variations in frequency and amplitude to when recorded with an established EEG system such as Enobio 8. However, recorded brain activity linked to upper limb motor-action and captured with EEGlass, displayed significant differences when compared to that captured with Enobio 8, as anticipated due to the localized motor activity of the sensorimotor cortices under C3, C4 electrodes. Yet, EEGlass managed to capture ERD from its TP9 and TP10 electrodes, though with less power than Enobio 8 due to the low spatial resolution of the EEG signals on the scalp, relying on signal propagation to reach the remotely located EEGlass electrodes. Moreover, EEGlass was able to detect subtle eye movements in 4 basic directions, displaying an eye-tracking potential particularly useful for navigating in heads-up interfaces.

Undoubtedly, low sample size ($N=1$) and stationary experimental settings are significant limitations that we will address in followup studies. However, human skull and brain anatomy is universally homogeneous, and the eyewear/HMD form factor ensures a rather stable electrode contact, only somewhat influenced by movement. In future iterations, we will utilize prominent machine learning techniques for training algorithms to match input from EEGlass to that of established EEG systems, and test our prototype in user studies with actual HMDs. We believe a merger between EEG and HMDs bears an unprecedented potential to revolutionize human-machine interaction, facilitating touch-less input and greatly increasing human-machine communication throughput.

6 ACKNOWLEDGEMENTS

The authors acknowledge the financial support of the Swiss National Science Foundation (SNSF) under grant number: 184146 We would also like to thank Ph.D. student Octavio Marin Pardo for helping with the data acquisition.

REFERENCES

- [1] Hans Berger. 1933. Über das elektroencephalogramm des menschen. *European archives of psychiatry and clinical neuroscience* 98, 1 (1933), 231–254.
- [2] Guillermo Bernal, Tao Yang, Abhinandan Jain, and Pattie Maes. 2018. PhysioHMD: a conformable, modular toolkit for collecting physiological data from head-mounted displays. In *Proceedings of the 2018 ACM International Symposium on Wearable Computers*. ACM, 160–167.
- [3] Mark Billingham and Thad Starner. 1999. Wearable devices: new ways to manage information. *Computer* 32, 1 (1999), 57–64.
- [4] György Buzsáki and Andreas Draguhn. 2004. Neuronal oscillations in cortical networks. *science* 304, 5679 (2004), 1926–1929.
- [5] Robert A Connor. 2018. EEG glasses (electroencephalographic eyewear). US Patent 9,968,297.
- [6] Nathan E Crone, Diana L Miglioretti, Barry Gordon, and Ronald P Lesser. 1998. Functional mapping of human sensorimotor cortex with electrocorticographic spectral analysis. II. Event-related synchronization in the gamma band. *Brain: a journal of neurology* 121, 12 (1998), 2301–2315.
- [7] Arnaud Delorme and Scott Makeig. 2004. EEGLAB: an open source toolbox for analysis of single-trial EEG dynamics including independent component analysis. *Journal of neuroscience methods* 134, 1 (2004), 9–21.
- [8] Thalia Harmony, Thalia Fernández, Juan Silva, Jorge Bernal, Lourdes Díaz-Comas, Alfonso Reyes, Erzsébet Marosi, Mario Rodríguez, and Miguel Rodríguez. 1996. EEG delta activity: an indicator of attention to internal processing during performance of mental tasks. *International journal of psychophysiology* 24, 1-2 (1996), 161–171.
- [9] Wolfgang Klimesch. 1999. EEG alpha and theta oscillations reflect cognitive and memory performance: a review and analysis. *Brain research reviews* 29, 2-3 (1999), 169–195.
- [10] Dietrich Lehmann, PL Faber, Peter Achermann, Daniel Jeanmonod, Lorena RR Gianotti, and Diego Pizzagalli. 2001. Brain sources of EEG gamma frequency during volitionally meditation-induced, altered states of consciousness, and experience of the self. *Psychiatry Research: Neuroimaging* 108, 2 (2001), 111–121.
- [11] Ernst Niedermeyer and FH Lopes da Silva. 2005. *Electroencephalography: basic principles, clinical applications, and related fields*. Lippincott Williams & Wilkins.
- [12] Evangelos Niforatos and Mélodie Vidal. 2019. Effects of a Monocular Laser-Based Head-Mounted Display on Human Night Vision. In *Proceedings of the 10th Augmented Human International Conference 2019*. ACM, 31.

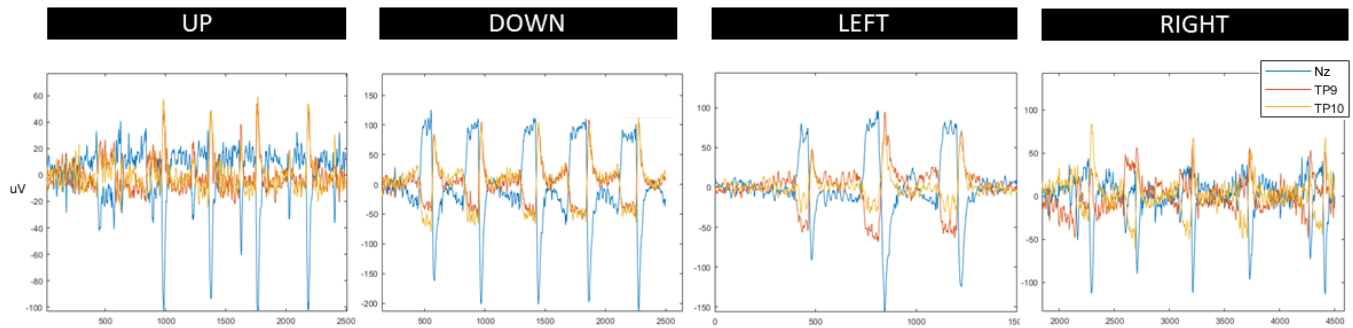


Figure 7: Electrooculographic (EOG) activity ($\mu\text{V}/\text{ms}$) recorded by EEGlass and linked to eye movement in 4 basic directions.

- [13] Evangelos Niforatos, Athanasios Vourvopoulos, and Marc Langheinrich. 2017. Amplifying human cognition: bridging the cognitive gap between human and machine. In *Proceedings of the 2017 ACM International Joint Conference on Pervasive and Ubiquitous Computing and Proceedings of the 2017 ACM International Symposium on Wearable Computers*. ACM, 673–680.
- [14] Gert Pfurtscheller and A Aranibar. 1979. Evaluation of event-related desynchronization (ERD) preceding and following voluntary self-paced movement. *Electroencephalography and clinical neurophysiology* 46, 2 (1979), 138–146.
- [15] Gert Pfurtscheller and Christa Neuper. 2001. Motor imagery and direct brain-computer communication. *Proc. IEEE* 89, 7 (2001), 1123–1134.
- [16] Gert Pfurtscheller, Christa Neuper, GR Muller, Bernhard Obermaier, Gunter Krausz, A Schlogl, Reinhold Scherer, Bernhard Graimann, Claudia Keinrath, Dimitris Skliris, et al. 2003. Graz-BCI: state of the art and clinical applications. *IEEE Transactions on neural systems and rehabilitation engineering* 11, 2 (2003), 1–4.
- [17] Yann Renard, Fabien Lotte, Guillaume Gibert, Marco Congedo, Emmanuel Maby, Vincent Delannoy, Olivier Bertrand, and Anatole Lécuyer. 2010. Openvibe: An open-source software platform to design, test, and use brain-computer interfaces in real and virtual environments. *Presence: teleoperators and virtual environments* 19, 1 (2010), 35–53.
- [18] Daniel L Schacter. 1977. EEG theta waves and psychological phenomena: A review and analysis. *Biological psychology* 5, 1 (1977), 47–82.
- [19] Dionisije Sopic, Amir Aminifar, and David Atienza. 2018. e-glass: A wearable system for real-time detection of epileptic seizures. In *2018 IEEE International Symposium on Circuits and Systems (ISCAS)*. IEEE, 1–5.
- [20] Yuji Uema and Kazutaka Inoue. 2017. JINS MEME algorithm for estimation and tracking of concentration of users. In *Proceedings of the 2017 ACM International Joint Conference on Pervasive and Ubiquitous Computing and Proceedings of the 2017 ACM International Symposium on Wearable Computers*. ACM, 297–300.
- [21] Athanasios Vourvopoulos and Sergi Bermudez i Badia. 2016. Usability and Cost-effectiveness in Brain-Computer Interaction: Is it User Throughput or Technology Related?. In *Proceedings of the 7th Augmented Human International Conference 2016*. ACM, 19.
- [22] Peter Welch. 1967. The use of fast Fourier transform for the estimation of power spectra: a method based on time averaging over short, modified periodograms. *IEEE Transactions on audio and electroacoustics* 15, 2 (1967), 70–73.